

OriGene Technologies, Inc.

9620 Medical Center Drive, Ste 200 Rockville, MD 20850, US Phone: +1-888-267-4436 https://www.origene.com techsupport@origene.com EU: info-de@origene.com CN: techsupport@origene.cn

Product datasheet for AM39011FC-N

CD8A Mouse Monoclonal Antibody [Clone ID: MCD8]

Product data:

Product Type:	Primary Antibodies
Clone Name:	MCD8
Applications:	FC
Recommended Dilution:	Flow cytometry: The reagent is effectively formulated for direct immunofluorescent staining (see "Protocols" below).
Reactivity:	Human
Host:	Mouse
lsotype:	lgG1
Clonality:	Monoclonal
Specificity:	The antibody detects the CD8 molecule, expressed as a heterodimer of CD8a (32-34 kD)and CD8b (32-34 kD) glycoproteins. Clone MCD8 is commonly used in routine immunophenotyping, the determination of CD4/CD8 ratios in HIV/AIDS patients and aids in the identification of T cell leukemias (common T-ALL or mature T-ALL)s. MCD8 also distinguishes between chronic B and T cell lymphoid leukemias.
Formulation:	0.01 M sodium phosphate, 0.15 M NaCl, pH 7.3, 0.2% BSA, 0.09% sodium azide Label: FITC State: Liquid purified Ig fraction
Purification:	Affinity chromatography
Conjugation:	FITC
Storage:	Store the antibody undiluted at 2-8°C. This product is photosensitive and should be protected from light.
Stability:	Shelf life: one year from despatch.
Gene Name:	CD8a molecule
Database Link:	<u>Entrez Gene 925 Human</u> <u>P01732</u>



This product is to be used for laboratory only. Not for diagnostic or therapeutic use. ©2024 OriGene Technologies, Inc., 9620 Medical Center Drive, Ste 200, Rockville, MD 20850, US


CD8 acts as a co-receptor with the TcR in recognizing antigens presented by MHC Class I and plays a role in the T cell-mediated immune response. The CD8 antigen is present on most tymocytes, T cytotoxic/suppressor cells and a subpopulation of NK cells. CD8 alpha chain, CD8A, MAL 1. Conjugates with brighter fluorochromes, like PE and APC, will have a greater separation than those with dyes like FITC. When populations overlap, the percentage of positive cells
1. Conjugates with brighter fluorochromes, like PE and APC, will have a greater separation than those with dyes like FITC. When populations overlap, the percentage of positive cells
than those with dyes like FITC. When populations overlap, the percentage of positive cells
using a selected marker can be affected by the choice of fluorescent label. 2. Use of monoclonal antibodies in patient treatment can interfere with antigen target recognition by this reagent. This should be taken into account when samples are analyzed from patients treated in this fashion. 3. Reagent data performance is based on EDTA-treated blood. Reagent performance can be affected by the use of other anticoagulants.
Protocol: <u>Flow cytometry method for use with labeled (FITC, R-PE, APC, PerCP or PerCP-Cy5.5</u>
 monoclonal antibodies 1. Add 100 µl of EDTA-treated blood (i.e. approx. 10e6 leukocytes) to a 5 ml reagent tube. The content of one tube is sufficient to perform one test. 2. Add to each tube 10 µl of labeled monoclonal antibody. (Appropriate mouse Ig isotype control samples should always be included in any labeling study). Vortex the tube to ensure thorough mixing of antibody and cells. 3. Incubate the tube for 15 minutes at room temperature in the dark. 4. Add 100 µl of a lyse reagent. 5. Incubate for 10 minutes at room temperature in the dark. 6. Add 2 ml of demineralized water and incubate for 10 minutes in the dark. 7. Centrifuge the labeled cell suspension for 2 minutes at 1000 x g. 8. Remove the supernatant and resuspend the cells in 200 µl of PBS. 9. Analyze by flow cytometry within four hours (alternatively, the cells may be fixed by 0.05% of formaline in buffered saline for analysis the next day. Some antigens are readily destroyed upon fixation and this should be taken into account when using this alternative).
 content of one tube is sufficient to perform one test. For combinations with anti-kappa and/or anti-lambda Ig see Application note below. 2. Add to each tube 20 µl of labeled monoclonal antibody combination. (Appropriate mouse Ig isotype control samples should always be included in any labeling study). 3. Vortex the tube to ensure thorough mixing of antibody and cells.
4. Incubate the tube for 15 minutes at room temperature in the dark. 5. Add 100 μl of a lyse reagent and mix immediately. 6. Incubate for 10 minutes at room temperature in the dark.

This product is to be used for laboratory only. Not for diagnostic or therapeutic use. ©2024 OriGene Technologies, Inc., 9620 Medical Center Drive, Ste 200, Rockville, MD 20850, US

	CD8A Mouse Monoclonal Antibody [Clone ID: MCD8] – AM39011FC-N
	9. Remove the supernatant and resuspend the cells in 200 μl of PBS. 10. Analyze by flow cytometry within four hours (alternatively, the cells may be fixed by 0.05% of formaline in buffered saline for analysis the next day. Some antigens are readily destroyed upon fixation and this should be taken into account when using this alternative).
	Application note for anti-kappa and/or anti-lambda lg combinations Add 2 ml of PBS containing 0.001% (v/v) Heparin (prewarmed to 37°C) to the cell suspension Vortex, centrifuge (2 min at 300x g) and discard the supernatant. Repeat this step twice. Resuspend the pelleted blood cells in 100 μl PBS, pH 7.2, containing 0.001% (v/v) Heparin.
Protein Families:	Adult stem cells, Druggable Genome, ES Cell Differentiation/IPS, Secreted Protein, Transmembrane
Protein Pathway	s: Antigen processing and presentation, Cell adhesion molecules (CAMs), Hematopoietic cell lineage, Primary immunodeficiency, T cell receptor signaling pathway

Product images:

ו// __

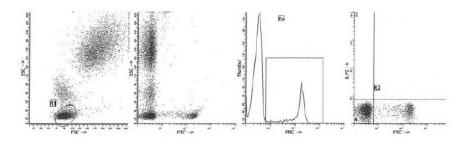

Staining with clone MCD8 (CD8) monoclonal antibody is illustrated by flow cytometry analysis of normal blood cells. Direct staining was performed using 10 μ l of the FITC-conjugated antibody and 100 μ l blood sample. Testing by flow cytometry using a 'lyse-wash' method on whole blood from healthy donors showed the following values expressed in terms of % of the total lymphocyte count: Product code: AM39011FC-N (anti-CD8 FITC) n: 10 Mean % positive: 26, 21 S.D.: 4, 55 % CV: 17, 36

This product is to be used for laboratory only. Not for diagnostic or therapeutic use. ©2024 OriGene Technologies, Inc., 9620 Medical Center Drive, Ste 200, Rockville, MD 20850, US