

## Human MMP13/Collagenase 3 ELISA Kit

**Catalog Number:** EA100326

### Assay Principle

The OriGene Human MMP13 Pre-Coated ELISA (Enzyme-Linked Immunosorbent Assay) kit is a solid phase immunoassay specially designed to measure Human MMP13 with a 96-well strip plate that is pre-coated with antibody specific for MMP13. The detection antibody is a biotinylated antibody specific for MMP13. The capture antibody is a polyclonal antibody from goat, the detection antibody is polyclonal antibody from goat. The kit contains recombinant Human MMP13 with immunogen: Expression system for standard: NSOi; Immunogen sequence: L20-C471. The kit is analytically validated with ready to use reagents.

To measure Human MMP13, add standards and samples to the wells, then add the biotinylated detection antibody. Wash the wells with PBS or TBS buffer, and add Avidin-Biotin-Peroxidase Complex (ABC-HRP). Wash away the unbound ABC-HRP with PBS or TBS buffer and add TMB. TMB is substrate to HRP and will be catalyzed to produce a blue color product, which changes into yellow after adding acidic stop solution. The density of the yellow product is linearly proportional to Human MMP13 in the sample. Read the density of the yellow product in each well using a plate reader, and benchmark the sample wells' readings against the standard curve to determine the concentration of Human MMP13 in the sample.

### Overview

<b>Product Name</b>	Human MMP13/Collagenase 3 ELISA
<b>Reactive Species</b>	Human
<b>Size</b>	96wells/kit, with removable strips.
<b>Description</b>	Sandwich High Sensitivity ELISA kit for Quantitative Detection of Human TGFB3. 96wells/kit, with removable strips.
<b>Sensitivity</b>	<5 pg/ml *The sensitivity or the minimum detectable dose (MDD) is the lower limit of target protein that can be detected by the kit. It is determined by adding two standard deviations to the mean O.D. value of twenty (20) blank wells and calculating the corresponding concentration.
<b>Detection Range</b>	156 pg/ml – 10.000 pg/ml
<b>Storage Instructions</b>	Store at 4°C for 6 months, at -20°C for 12 months. Avoid multiple freeze-thaw cycles (Shipped with wet ice.)
<b>Uniprot ID</b>	P45452

## Technical Details

<b>Capture/Detection Antibodies</b>	The capture antibody is polyclonal antibody from goat, the detection antibody is polyclonal antibody from goat.
<b>Specificity</b>	Natural and recombinant Human MMP13
<b>Immunogen</b>	Expression system for standard: NSO; Immunogen Sequence: L20-C471
<b>Cross Reactivity</b>	There is no detectable cross-reactivity with other relevant proteins.

## Notice Before Application

Please read the following instructions before starting the experiment.

1. To inspect the validity of experiment operation and the appropriateness of sample dilution proportion, pilot experiment using standards and a small number of samples is recommended.
2. Before using the Kit, spin tubes and bring down all components to the bottom of tubes.
3. Don't let 96-well plate dry, for dry plate will inactivate active components on plate.
4. Don't reuse tips and tubes to avoid cross contamination.
5. Avoid using the reagents from different batches together.

## Kit Components/Materials Provided

Description	Quantity	Volume
Anti-Human MMP13 Pre-coated 96-well strip microplate	1	12 strips of 8 wells
Human MMP13 Standard	2	10 ng/tube
Human MMP13 Biotinylated antibody (100x)	1	100 $\mu$ l
Avidin-Biotin-Peroxidase Complex (100x)	1	100 $\mu$ l
Sample Diluent	1	30ml
Antibody Diluent	1	12ml
Avidin-Biotin-Peroxidase Diluent	1	12ml
Color Developing Reagent (TMB)	1	10ml
Stop Solution	1	10ml
Plate Sealers	4	Piece
Wash Buffer(25x)	1	20 ml

## Required Materials That Are Not Supplied

Microplate Reader capable of reading absorbance at 450nm.

Automated plate washer (optional)

Pipettes and pipette tips capable of precisely dispensing 0.5  $\mu$ l through 1 ml volumes of aqueous solutions. Multichannel pipettes are recommended for large amount of samples.

Deionized or distilled water.

500ml graduated cylinders.


Test tubes for dilution.

## Human MMP13 ELISA Kit (EA100326) Standard Curve Example

Highest O.D. value might be higher or lower than in the example. The experiment result is statistically significant if the highest O.D. value is no less than 1.0.

Concentration (pg/ml)	0	156	312	625	1250	2500	5000	10.000
O.D.	0.121	0.230	0.347	0.542	0.838	1.249	1.770	2.157

### Human MMP13 ELISA Kit standard curve

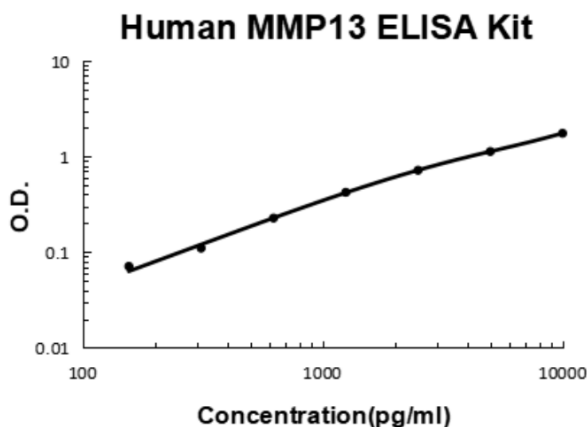

A standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

## Intra/Inter Assay Variability

OriGene spend great efforts in documenting lot to lot variability and make sure our assay kits produce robust data that are reproducible.

**Intra-Assay Precision (Precision within an assay):** Three samples of known concentration were tested on one plate to assess intra-assay precision.

**Inter-Assay Precision (Precision across assays):** Three samples of known concentration were tested in separate assays to assess inter-assay precision.

Sample	Intra-Assay Precision			Inter-Assay Precision		
	1	2	3	1	2	3
n	16	16	16	24	24	24
Mean(pg/ml)	219	1742	4482	203	1816	4413
Standard deviation	14.01	116.71	313.74	16.42	146.48	357.45
CV(%)	6.4 %	6.7 %	7 %	7.5 %	8 %	8.1 %

## Reproducibility

To assay reproducibility, three samples with differing target protein concentrations were assayed using four different lots.

Lots	Lot1 (pg/ml)	Lot2 (pg/ml)	Lot3 (pg/ml)	Lot4 (pg/ml)	Mean (pg/ml)	Standard Deviation	CV (%)
Sample 1	219	230	199	236	221	14.08	6.3%
Sample 2	1742	1734	1789	1510	1693	108.14	6.3 %
Sample 3	4482	4805	4585	4324	4549	174.6	3.8 %

\*number of samples for each test n=16.

## Preparation Before The Experiment

Item	Preparation
All reagents	<p>Bring all reagents to 37°C prior to use. The assay can also be done at room temperature however we recommend doing it at 37°C for best consistency with our QC results. Also the TMB incubation time estimate (15-25min) is based on 37°C.</p> <p>Do not equilibrate unused plate well strips to room temperature; these should be sealed and stored in the original packaging.</p>
Wash buffer	Prepare 500 ml of working Wash Buffer by diluting the supplied 20 ml of Wash Buffer (25x) with 480 ml of deionized or distilled water. If crystals have formed in the concentrate, warm to room temperature and mix it gently until crystals have completely dissolved.
Biotinylated Anti-Human MMP13 antibody	It is recommended to prepare this reagent immediately prior to use by diluting the Human MMP13 Biotinylated antibody (100x) 1:100 with Antibody Diluent. Prepare 100 µl by adding 1 µl of Biotinylated antibody (100x) to 99 µl of Antibody Diluent for each well. Mix gently and thoroughly and use within 2 hours of generation.
Avidin-Biotin-Peroxidase Complex	It is recommended to prepare this reagent immediately prior to use by diluting the Avidin-Biotin-Peroxidase Complex (100x) 1:100 with Avidin-Biotin-Peroxidase Diluent. Prepare 100 µl by adding 1 µl of Avidin-Biotin-Peroxidase Complex (100x) to 99 µl of Avidin-Biotin-Peroxidase Diluent for each well. Mix gently and thoroughly and use within 2 hours of generation.
Human MMP13 Standard	It is recommended that the standards be prepared no more than 2 hours prior to performing the

	experiment. Use one 10 ng of lyophilized Human MMP13 standard for each experiment. Gently spin the vial prior to use. Reconstitute the standard to a stock concentration of 10 ng/ml using 1 ml of sample diluent. Allow the standard to sit for a minimum of 10 minutes with gentle agitation prior to making dilutions.
Microplate	The included microplate is coated with capture antibodies and ready-to-use. It does not require additional washing or blocking. The unused well strips should be sealed and stored in the original packaging.

## Dilution of Human MMP13 Standard

1. Number tubes 1-8. Final Concentrations to be Tube # 1 - 10,000 pg/ml, # 2 - 5000 pg/ml, # 3 - 2500 pg/ml, # 4 - 1250 pg/ml, # 5 - 625 pg/ml, # 6 - 312.50 pg/ml, # 7 - 165.25 pg/ml, # 8 - 0.0 (Blank - Sample diluent serves as the zero standard).
2. To generate standard # 1, add 1000  $\mu$ l of the reconstituted standard stock solution to tube # 1.
3. Add 300  $\mu$ l of sample diluent to tubes # 2-7.
4. To generate standard # 2, add 300  $\mu$ l of standard # 1 from tube # 1 to tube # 2 for a final volume of 600  $\mu$ l. Mix thoroughly.
5. To generate standard # 3, add 300  $\mu$ l of standard # 2 from tube # 2 to tube # 3 for a final volume of 600  $\mu$ l. Mix thoroughly.
6. Continue the serial dilution for tube # 4-7.
7. Tube # 8 is a blank standard to be used with every experiment.

## Sample Preparation and Storage

These sample collection instructions and storage conditions are intended as a general guideline and the sample stability has not been evaluated.

Sample Type	Procedure
Cell culture supernatants	Clear sample of particulates by centrifugation, assay immediately or store samples at -20°C.
Serum	Use a serum separator tube (SST) and allow serum to clot at room temperature for about four hours. Then, centrifuge for 15 min at approximately 1,000 xg. assay immediately or store samples at -20°C.
Plasma	Collect plasma using heparin as an anticoagulant. Centrifuge for 15 min at approximately 1,000 xg. assay immediately or store samples at -20°C. Note: it is important to not use anticoagulants other than the ones described above to treat plasma for other anticoagulants could block the antibody binding site.

## Sample Collection Notes

1. It is recommended to use the samples immediately upon preparation.
2. Avoid repeated freeze/thaw cycles for all samples.
3. In the event that a sample type not listed above is intended to be used with the kit, it is recommended that the customer conduct validation experiments in order to be confident in the results.
4. Due to chemical interference, the use of tissue or cell extraction samples prepared by chemical lysis buffers may result in inaccurate results.
5. Due to factors including cell viability, cell number, or sampling time, samples from cell culture supernatant may not be detected by the kit.
6. Samples should be brought to room temperature (18-25°C) before performing the assay without the use of extra heating.

7. Sample concentrations should be predicted before being used in the assay. If the sample concentration is not within the range of the standard curve, users must determine the optimal sample dilutions for their particular experiments.

## Sample Dilution

The target protein concentration should be estimated and appropriate sample dilutions should be selected such that the final protein concentration lies near the middle of the linear dynamic range of the assay.

It is recommended to prepare 150  $\mu$ l of sample for each replicate to be assayed. The samples should be diluted with sample diluent and mixed gently.

## Assay protocol

It is recommended that all reagents and materials be equilibrated to 37°C/room temperature prior to the experiment (see Preparation Before The Experiment if you have missed this information).

1. Prepare all reagents and working standards as directed previously.
2. Remove excess microplate strips from the plate frame and seal and store them in the original packaging.
3. Add 100  $\mu$ l of the standard, samples, or control per well. Add 100  $\mu$ l of the sample diluent buffer into the control well (Zero well). At least two replicates of each standard, sample, or control is recommended.
4. Cover with the plate sealer provided and incubate for 120 minutes at RT (or 90 min. at 37 °C).
5. Remove the cover and discard the liquid in the wells into an appropriate waste receptacle. Invert the plate on the benchtop onto a paper towel and tap the plate to gently blot any remaining liquid. It is recommended that the wells are not allowed to completely dry at any time.
6. Add 100  $\mu$ l of the prepared 1x Biotinylated Anti-Human MMP13 antibody to each well.
7. Cover with plate sealer and incubate for 90 minutes at RT (or 60 minutes at 37°C).
8. Wash the plate 3 times with the 1x wash buffer.
  - a. Discard the liquid in the wells into an appropriate waste receptacle. Then, invert the plate on the benchtop onto a paper towel and tap the plate to gently blot any remaining liquid. It is recommended that the wells are not allowed to completely dry at any time.
  - b. Add 300  $\mu$ l of the 1x wash buffer to each assay well. (For cleaner background incubate for 60 seconds between each wash).
  - c. Repeat steps a-b 2 additional times.
9. Add 100  $\mu$ l of the prepared 1x Avidin-Biotin-Peroxidase Complex into each well. Cover with the plate sealer provided and incubate for 40 minutes at RT (or 30 minutes at 37°C).
10. Wash the plate 5 times with the 1x wash buffer.
  - a. Discard the liquid in the wells into an appropriate waste receptacle. Then, invert the plate on the benchtop onto a paper towel and tap the plate to gently blot any remaining liquid. It is recommended that the wells are not allowed to completely dry at any time.
  - b. Add 300  $\mu$ l of the 1x wash buffer to each assay well. (For cleaner background incubate for 60 seconds between each wash).
  - c. Repeat steps a-b 4 additional times.
11. Add 90  $\mu$ l of Color Developing Reagent to each well. Cover with the plate sealer provided and incubate in the dark for 30 minutes at RT (or 15-25 minutes at 37°C). (The optimal incubation time must be empirically determined. A guideline to look for is blue shading the top four standard wells, while the remaining standards remain clear.)
12. Add 100  $\mu$ l of Stop Solution to each well. The color should immediately change to yellow.
13. Within 30 minutes of stopping the reaction, the O.D. absorbance should be read with a microplate reader at 450nm.

## Data Analysis

Average the duplicate readings for each standard, sample, and control. Subtract the average zero standard O.D. reading.

It is recommended that a standard curve be created using computer software to generate a four parameter logistic (4-PL) curve-fit. A free program capable of generating a four parameter logistic (4-PL) curve-fit can be found online at: [www.myassays.com/four-parameter-logistic-curve.assay](http://www.myassays.com/four-parameter-logistic-curve.assay)

Alternatively, plot the mean absorbance for each standard against the concentration. The measured concentration in the sample can be interpolated by using linear regression of each average relative OD against the standard curve generated using curve fitting software. This will generate an adequate but less precise fit of the data.

For diluted samples, the concentration reading from the standard curve must be multiplied by the dilution factor.

## Background on MMP13

Collagenase 3 is an enzyme that in humans is encoded by the MMP13 gene. <sup>1,2</sup> Most MMP's are secreted as inactive proproteins which are activated when cleaved by extracellular proteinases. The protein encoded by this gene cleaves type II collagen more efficiently than types I and III. The expression of MMP13 in osteoarthritic cartilage and its activity against type II collagen indicates that the enzyme plays a significant role in cartilage collagen degradation and must, therefore, form part of a complex target for proposed therapeutic interventions based on collagenase inhibition. It may be involved in articular cartilage turnover and cartilage pathophysiology associated with osteoarthritis. The gene is part of a cluster of MMP genes which localize to chromosome 11q22.3.

### Reference

1. Freije JM, Diez-Itza I, Balbin M, Sanchez LM, Blasco R, Tolivia J, Lopez-Otin C (Jul 1994). "Molecular cloning and expression of collagenase-3, a novel human matrix metalloproteinase produced by breast carcinomas". *J Biol Chem* 269 (24): 16766-73.
2. "Entrez Gene: MMP13 matrix metalloproteinase 13 (collagenase 3)".