

Product datasheet for **TL314710**

Aquaporin 5 (AQP5) Human shRNA Plasmid Kit (Locus ID 362)

Product data:

Product Type:	shRNA Plasmids
Product Name:	Aquaporin 5 (AQP5) Human shRNA Plasmid Kit (Locus ID 362)
Locus ID:	362
Synonyms:	AQP-5; PPKB
Vector:	pGFP-C-shLenti (TR30023)
E. coli Selection:	Chloramphenicol (34 ug/ml)
Mammalian Cell Selection:	Puromycin
Format:	Lentiviral plasmids
Components:	AQP5 - Human, 4 unique 29mer shRNA constructs in lentiviral GFP vector(Gene ID = 362). 5µg purified plasmid DNA per construct 29-mer scrambled shRNA cassette in pGFP-C-shLenti Vector, TR30021, included for free.
RefSeq:	NM_001651 , NM_001651.2 , NM_001651.3 , BC032946 , BC032946.1 , NM_001651.4
UniProt ID:	P55064
Summary:	Aquaporin 5 (AQP5) is a water channel protein. Aquaporins are a family of small integral membrane proteins related to the major intrinsic protein (MIP or AQP0). Aquaporin 5 plays a role in the generation of saliva, tears and pulmonary secretions. AQP0, AQP2, AQP5, and AQP6 are closely related and all map to 12q13. [provided by RefSeq, Jul 2008]
shRNA Design:	These shRNA constructs were designed against multiple splice variants at this gene locus. To be certain that your variant of interest is targeted, please contact techsupport@origene.com . If you need a special design or shRNA sequence, please utilize our custom shRNA service .




[View online »](#)


**Performance
Guaranteed:**

OriGene guarantees that the sequences in the shRNA expression cassettes are verified to correspond to the target gene with 100% identity. One of the four constructs at minimum are guaranteed to produce 70% or more gene expression knock-down provided a minimum transfection efficiency of 80% is achieved. Western Blot data is recommended over qPCR to evaluate the silencing effect of the shRNA constructs 72 hrs post transfection. To properly assess knockdown, the gene expression level from the included scramble control vector must be used in comparison with the target-specific shRNA transfected samples.


For non-conforming shRNA, requests for replacement product must be made within ninety (90) days from the date of delivery of the shRNA kit. To arrange for a free replacement with newly designed constructs, please contact Technical Services at techsupport@origene.com. Please provide your data indicating the transfection efficiency and measurement of gene expression knockdown compared to the scrambled shRNA control (Western Blot data preferred).

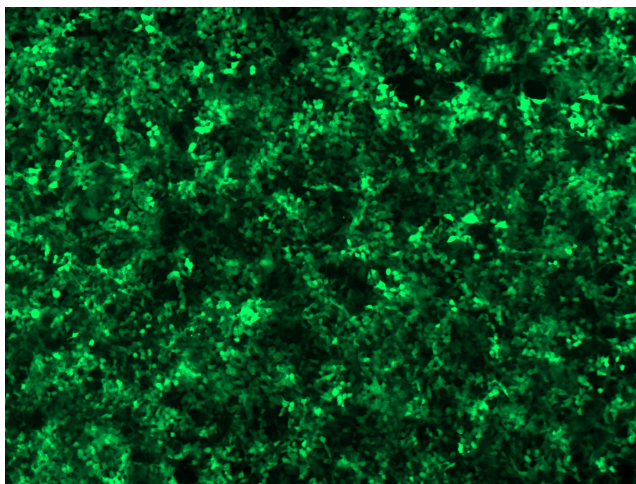Product images:


GFP signal was observed under microscope at 48 hours after transduction of TL314710A virus into HEK293 cells. TL314710A virus was prepared using lenti-shRNA TL314710A and [TR30037] packaging kit.

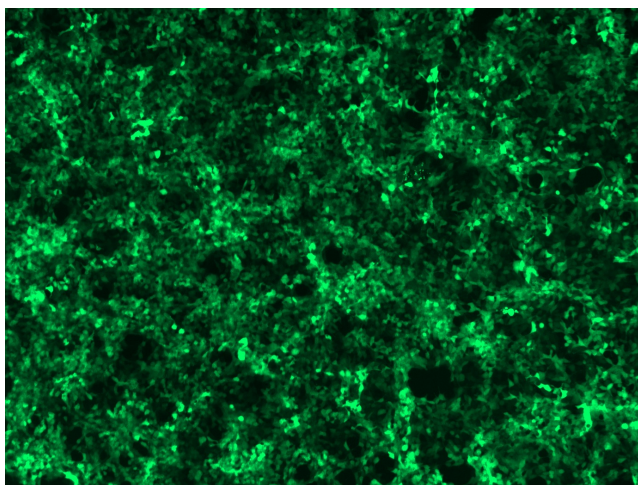

GFP signal was observed under microscope at 48 hours after transduction of TL314710B virus into HEK293 cells. TL314710B virus was prepared using lenti-shRNA TL314710B and [TR30037] packaging kit.

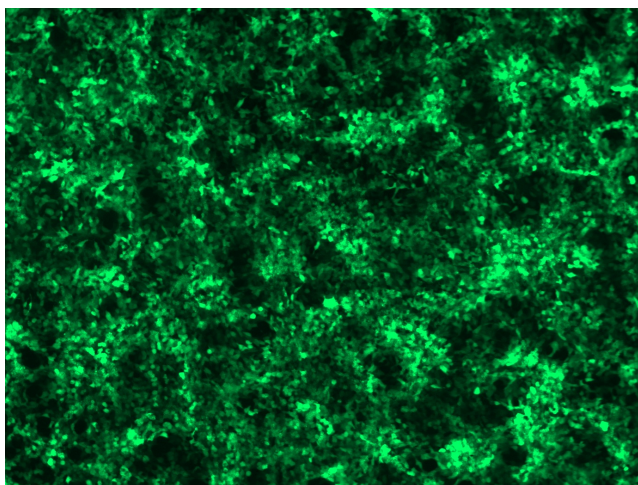

GFP signal was observed under microscope at 48 hours after transduction of [TL314710C] virus into HEK293 cells. [TL314710C] virus was prepared using lenti-shRNA [TL314710C] and [TR30037] packaging kit.

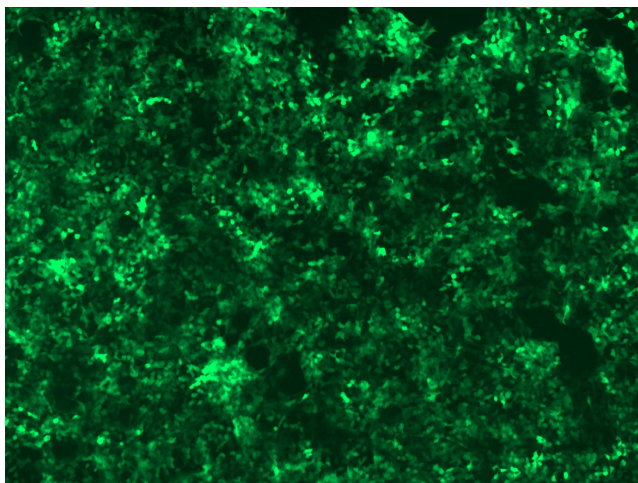

GFP signal was observed under microscope at 48 hours after transduction of [TL314710D] virus into HEK293 cells. [TL314710D] virus was prepared using lenti-shRNA [TL314710D] and [TR30037] packaging kit.